
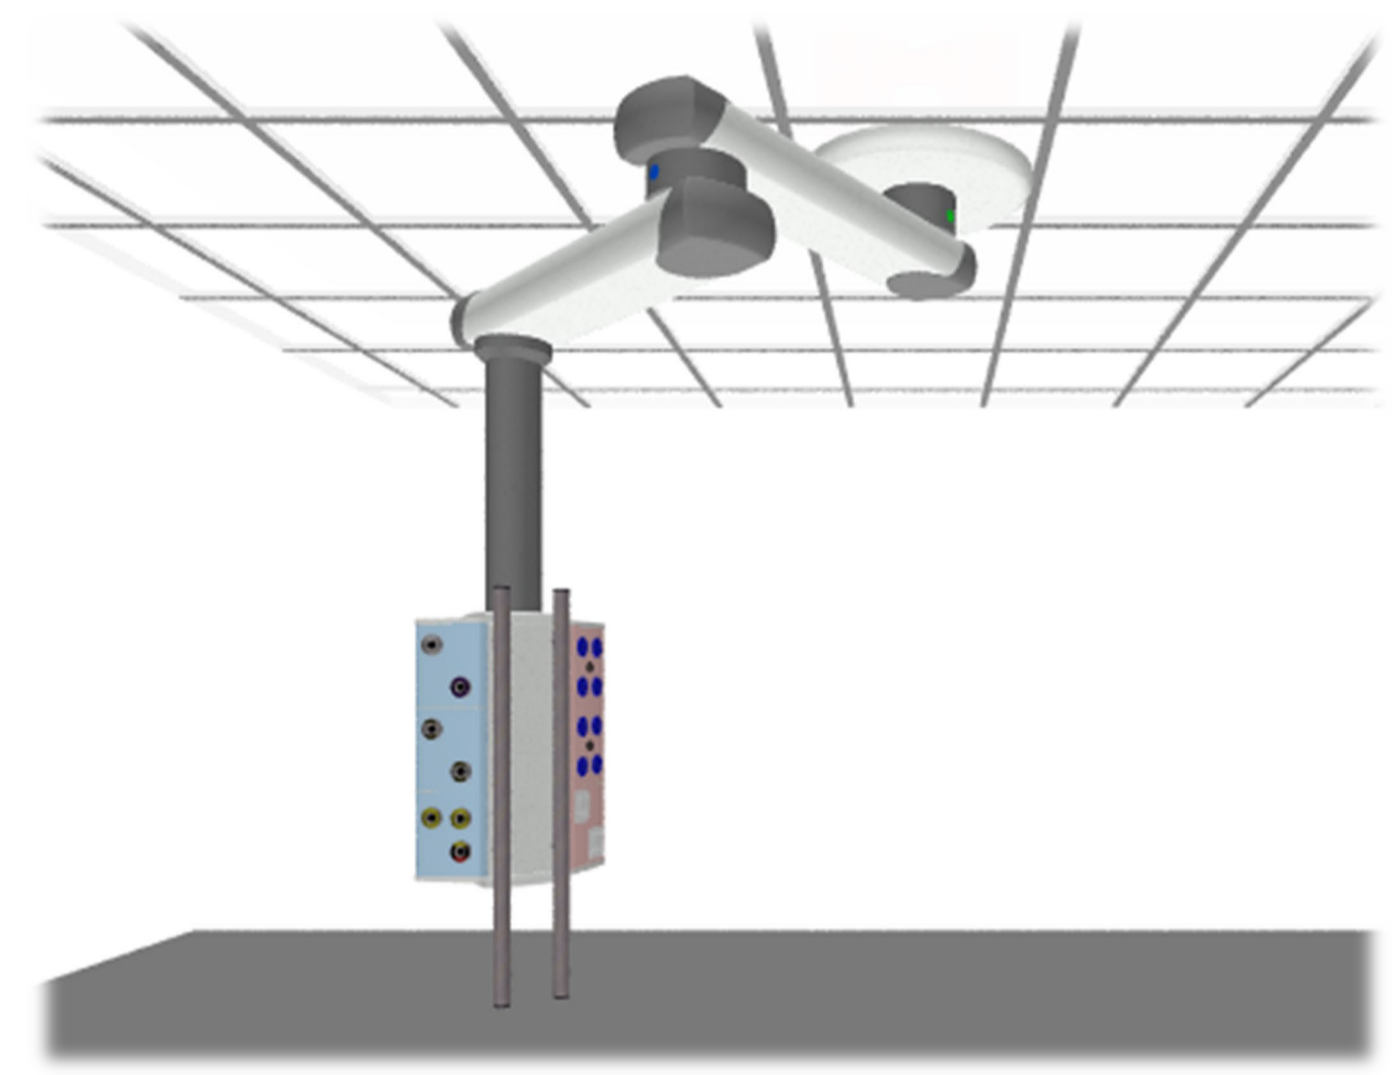


Surgeons Pendant – HBN26 Compliant

DATE	MODIFICATION	SIGN	ISSUE

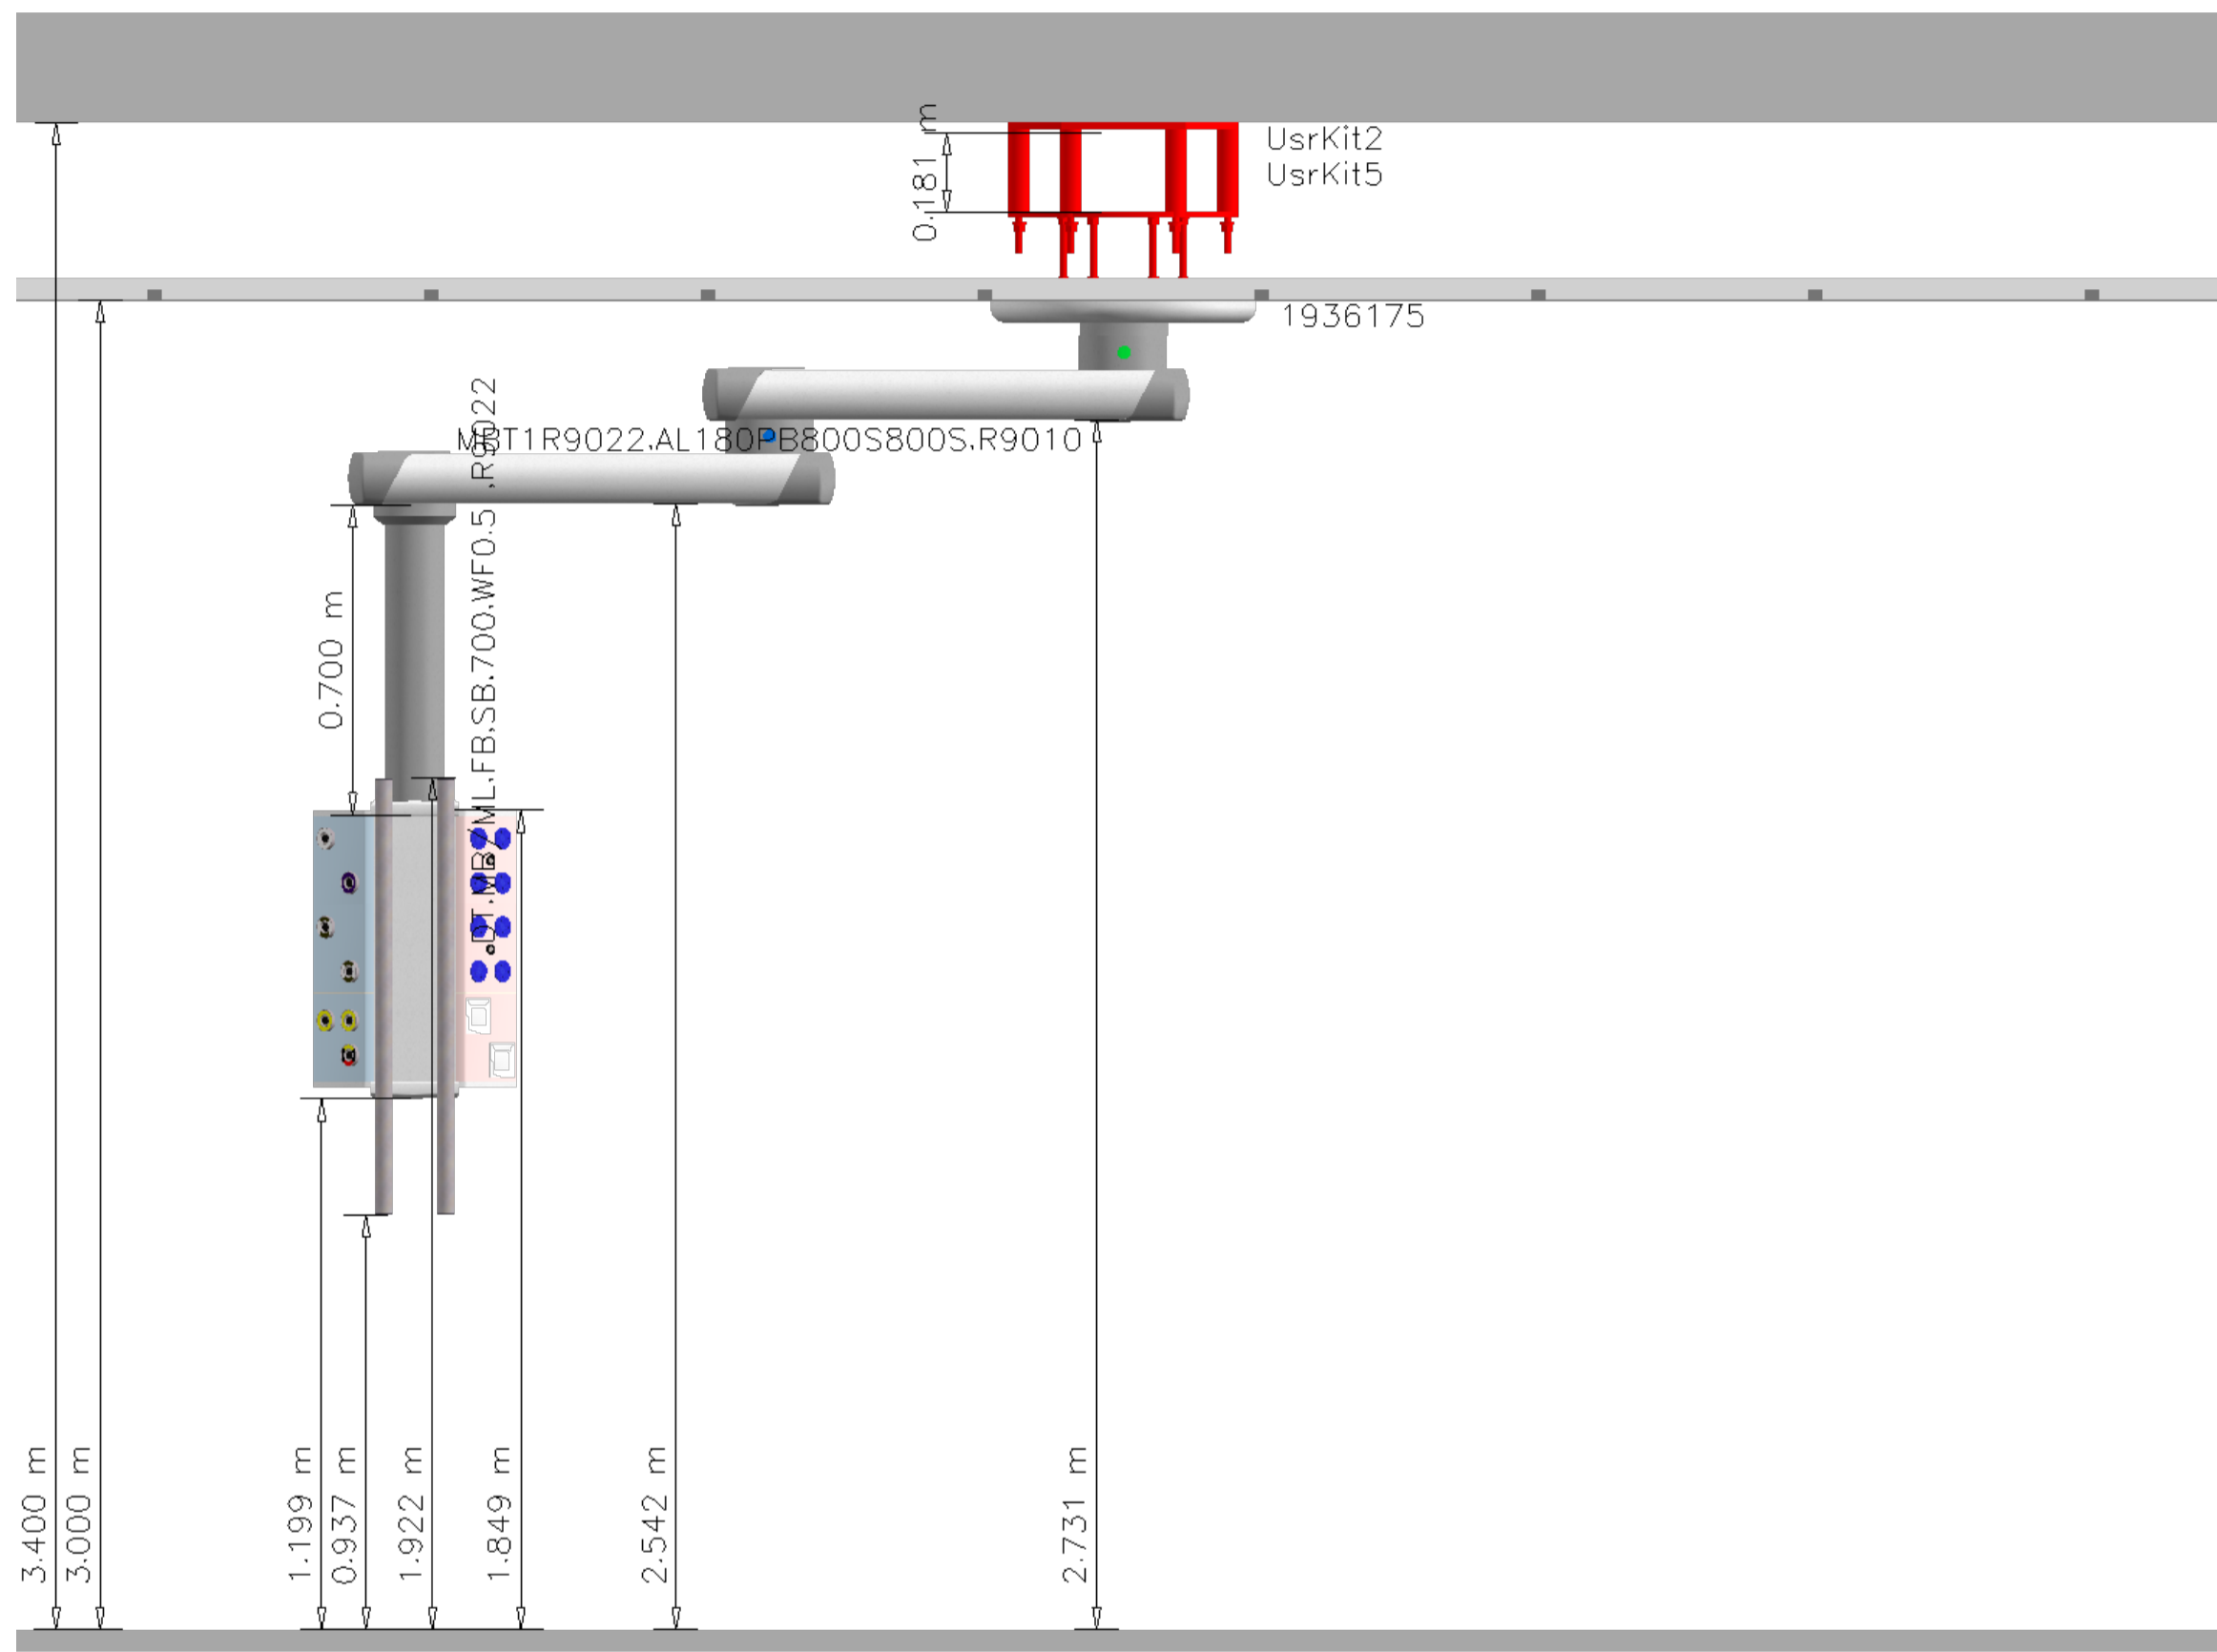


Brandon Atlas Anaesthetists Pendant Specification

1st Fix Assembly
 Cavity Spacer Kit ≤1000mm (to span void to 1200mm) incorporates upper plate for fixing to structural ceiling & intermediate Ceiling Plate which supports the Medical Gas & Suction NIST Connections & LV Electrical Connection Box (included).

Multi-Movement Arms
 800mm/800mm Lateral Movement Arms with Electromagnetic Brakes
 LED Lightguide brake release indication on all points of Arm Rotation

Service Head
 600mm M6 Service Head
 Service Head is provided pre-installed and tested with indicated services.

System Weights & Payloads.
 Overall Weight of the Configuration: 165 kg
 Vertical force as configured: 3016 N
 Max. Pendant Pay Load: 180 kg
 Remaining Net Pay Load: 142 kg
 Remaining Diameter, Left Arm: 53 %

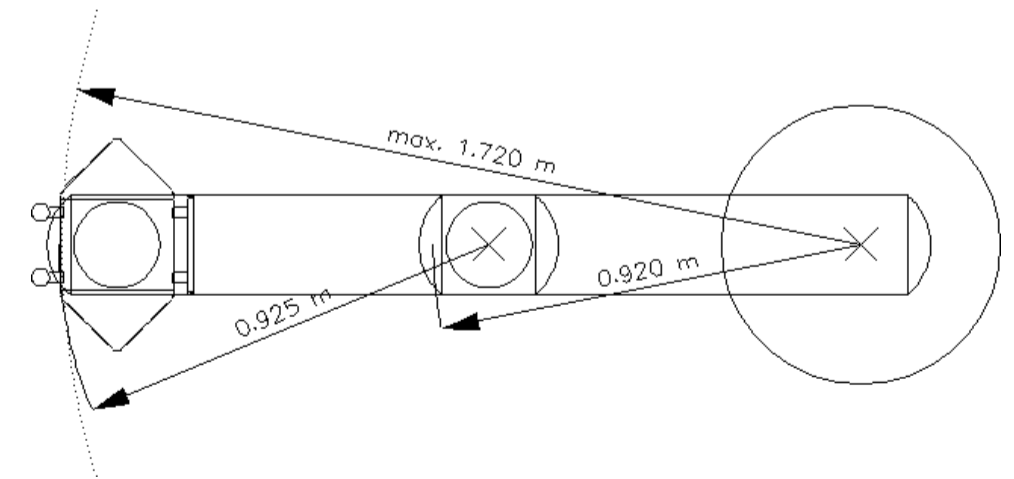

Creation Date	2020
Revision	
Author	PMG
CAD	OPM
Scale	Not To Scale
Sheet Size	A4


Status of Drawings
 Sales drawings are intended to enable customers to understand the design methodology and assess proposals for competitive tenders. Sales and tender drawings shall not be used as an installation drawing unless specifically agreed in the contract.
Warning
 Do not scale. All drawings issued pre-contract are subject to change and approval. Project drawings will be issued under the control of Brandon Medical Co Ltd quality assurance systems.
Checking
 This drawing has been generated using a Computer Aided Design system. As the system generates a new drawing at each revision, only the latest edition will have been initialled as checked.

For the Client:	
For the attention of:	
Contract	

Sample Surgeons Pendant – HBN26 Compliant			
Drawing Reference No.		Job Reference No.	
		Customer Sign Off	

Surgeons Pendant – HBN26 Compliant

DATE	MODIFICATION	SIGN	ISSUE

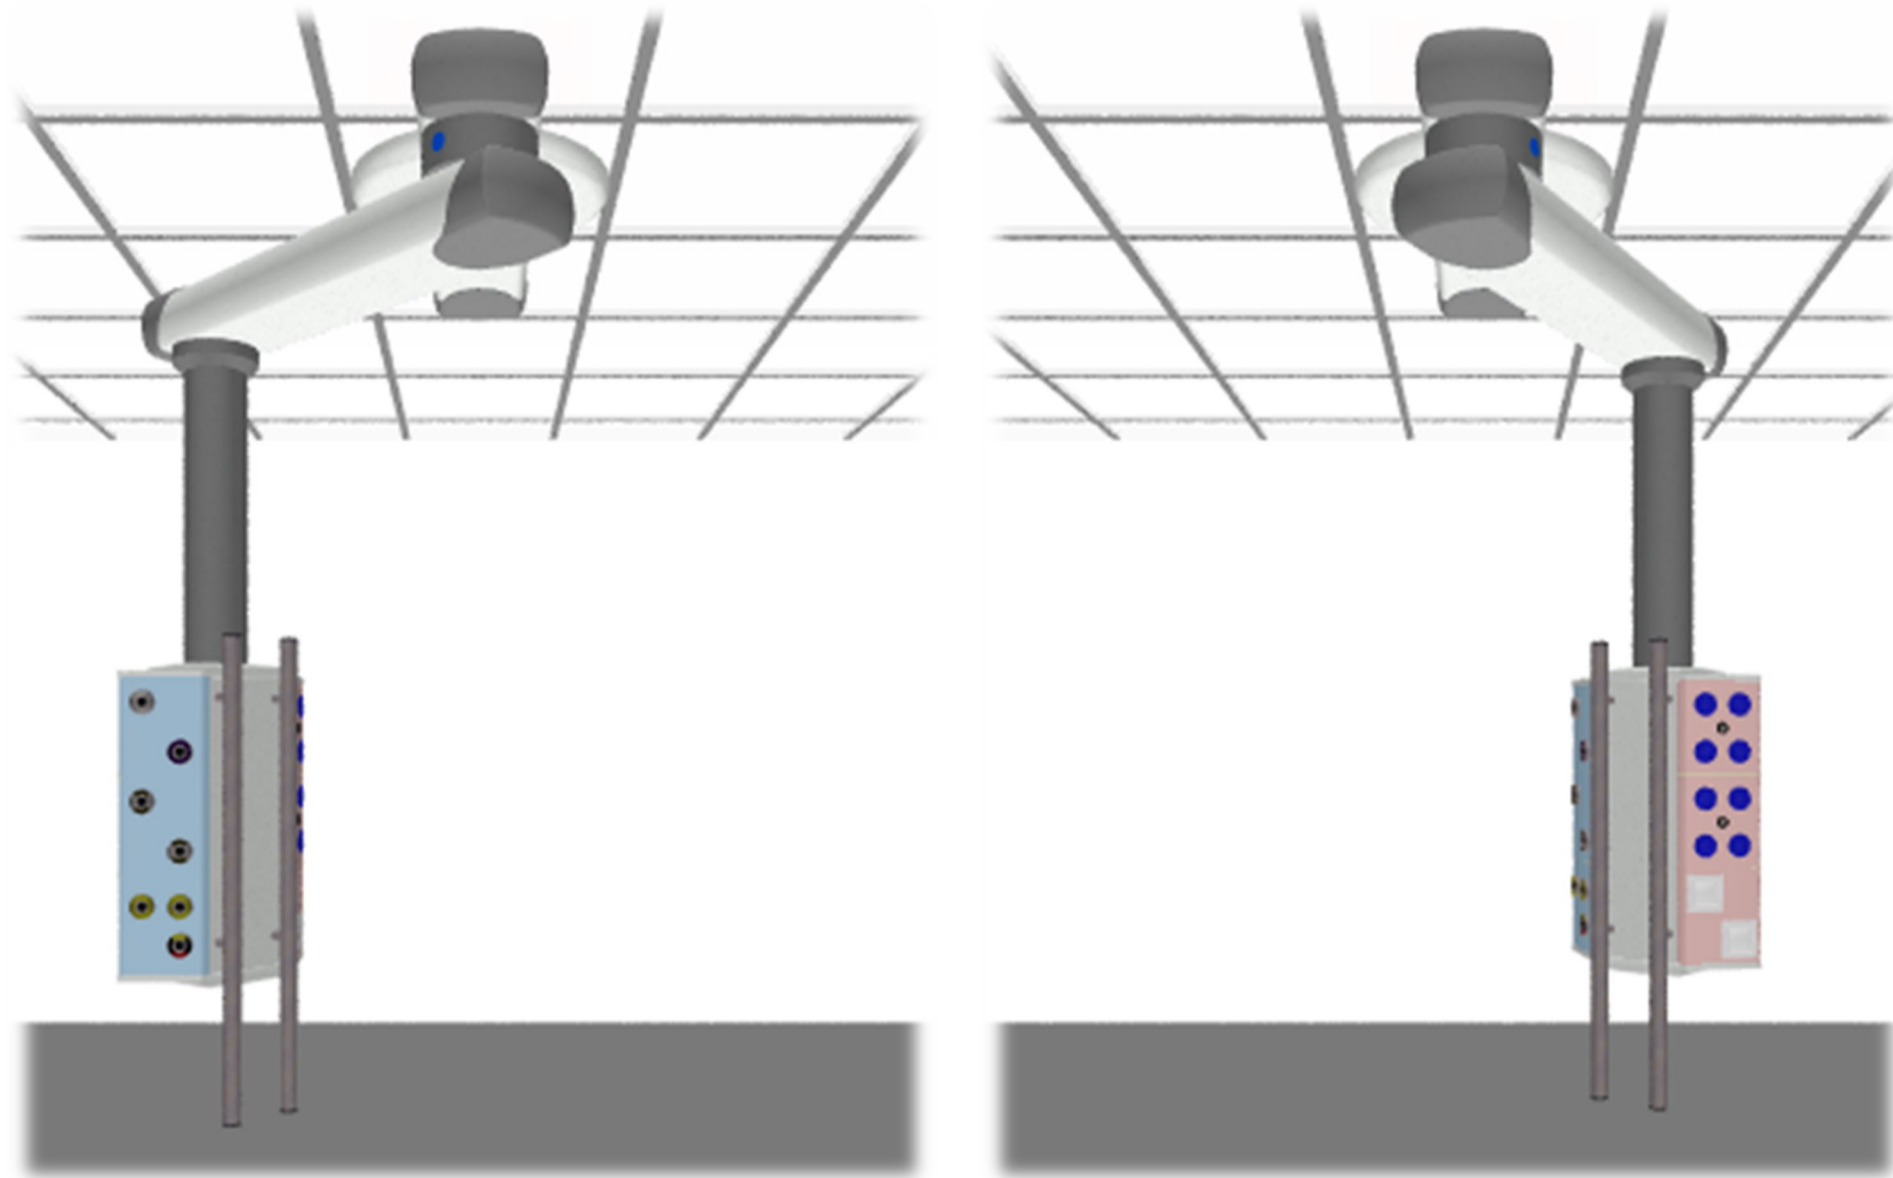

Service Head Specification

- 600mm M6 Service head
- 1000mm Multifunction rack to front face for accessory mounting
- Handle with brake controls to rear face

Pre Installed Service Outlets

12 No. 240V 13 A Electrical Outlets BS7671 and HTM06-01 Compliant

6 No. Single Gang Provision

- 1 No. Medical Oxygen Terminal Unit
- 1 No. Nitrous Oxide Terminal Unit
- 1 No. Medical Air 4 Bar Terminal Units
- 1 No. Surgical Air 7 bar Terminal Unit
- 2 No. Medical Vacuum Terminal Units
- 1 No. AGSS Terminal Unit

Medical Gas & Vacuum Terminal Units British Standard to BS EN ISO 9170-2-2008



ELMFIELD ROAD, MORLEY, LEEDS
LS27 0EL, UNITED KINGDOM
TELEPHONE: +44 (0)113 277 7393
FAX: +44 (0)113 272 8844
E-MAIL: enquiries@brandon-medical.com
WEB: www.brandon-medical.com

This drawing is copyright and may be reproduced, altered or used for any purpose other than that for which it is issued without the written permission of Brandon Medical Co Ltd. Any drawings, design information, guidance or product selections provided by Brandon Medical Co Ltd are given without responsibility or liability other than for incorporating into an order for Brandon Medical Co Ltd to execute works. Drawings are provided for guidance only and do not constitute final design authority.

Creation Date	2020
Revision	
Author	PMG
CAD	OPM
Scale	Not To Scale
Sheet Size	A4

Status of Drawings
Sales drawings are intended to enable customers to understand the design methodology and assess proposals for competitive tenders. Sales and tender drawings shall not be used as an installation drawing unless specifically agreed in the contract.
Warning
Do not scale. All drawings issued pre-contract are subject to change and approval. Project drawings will be issued under the control of Brandon Medical Co Ltd quality assurance systems.
Checking
This drawing has been generated using a Computer Aided Design system. As the system generates a new drawing at each revision, only the latest edition will have been initialled as checked.

For the Client:	
For the attention of:	
Contract	

Sample Surgeons Pendant – HBN26 Compliant	
Drawing Reference No.	
Job Reference No.	
Customer Sign Off	